Instruction Manual

Model 2115-275-1845

Block Upconverter

July 2017, Rev. 0



Data, drawings, and other material contained herein are proprietary to Cross Technologies, Inc., but may be reproduced or duplicated without the prior permission of Cross Technologies, Inc. for purposes of operating the equipment.

When ordering parts from Cross Technologies, Inc., be sure to include the equipment model number, equipment serial number, and a description of the part.



6170 Shiloh Road Alpharetta, Georgia 30005

(770) 886-8005 FAX (770) 886-7964 Toll Free 888-900-5588

WEB www.crosstechnologies.com E-MAIL info@crosstechnologies.com

INSTRUCTION MANUAL

MODEL 2115-275-1845 Block Upconverter

TABLE OF CONTENTS	PAGE
Warranty	2
1.0 General	3
1.1 Equipment Description	3
1.2 Technical Characteristics	4
2.0 Installation	5
2.1 Mechanical	5
2.2 Rear Inputs and Outputs	6
2.3 Front Panel Indicators	6
2.4 Operation	7
2.5 Environmental Use Information	8

WARRANTY - The following warranty applies to all Cross Technologies, Inc. products.

All Cross Technologies, Inc. products are warranted against defective materials and workmanship for a period of one year after shipment to customer. Cross Technologies, Inc.'s obligation under this warranty is limited to repairing or, at Cross Technologies, Inc.'s option, replacing parts, subassemblies, or entire assemblies. Cross Technologies, Inc. shall not be liable for any special, indirect, or consequential damages. This warranty does not cover parts or equipment which have been subject to misuse, negligence, or accident by the customer during use. All shipping costs for warranty repairs will be prepaid by the customer. There are not other warranties, express or implied, except as stated herein.



6170 Shiloh Road Alpharetta, Georgia 30005

(770) 886-8005 FAX (770) 886-7964 Toll Free 888-900-5588

WEB www.crosstechnologies.com E-MAIL info@crosstechnologies.com

MODEL 2115-275-1845 Block Upconverter

1.0 General

1.1 Equipment Description

The 2115-275-1845 Block Upconverter converts 1.345 - 2.345 GHz (Fc=1845 MHz) to 27.50 - 28.50 GHz with a local oscillator at 26.155 GHz. Front panel LEDs provide indication of DC Power, External 10 MHz, and PLL Alarm. The gain is +20 dB. Connectors are 2.92 mm female for the RF out and BNC female for the RF in (desgnated L-Band) and external reference input and reference output. A three-way switch controls which 10 MHz reference is being used. In the INT position, the internal reference is used, in the EXT position, the external reference is used, and in the AUTO position, the internal reference is used unless a +3 dBm ± 3 dB, 10MHz reference signal is connected to the external reference input. It is powered by a $100-240 \pm 10\%$ VAC power supply, and in a 1.3/4° X 19° X 14° rack mount chassis

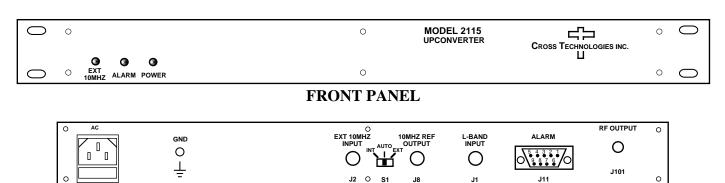


FIGURE 1.1 Model 2115-275-1845 Front and Rear Panels

REAR PANEL

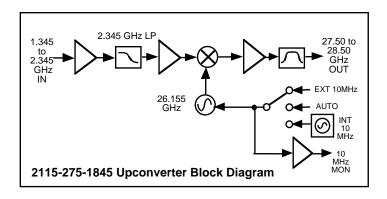


FIGURE 1.2 Model 2115-275-1845 Upconverter Block Diagram


1.2 Technical Characteristics

845 Block Upconverter Specifications*		
eated L-Band)		
50Ω / 14 dB		
1.345 to 2.345 GHz		
20 dB maximum gain		
-40 to -25 dBm		
-15 dBm		
50Ω / 14 dB		
27.50 to 28.50 GHz		
-20 to -5 dBm		
+5 dBm		
1		
+ 20 ± 1 dB at Fc		
> 60 dB, minimum		
SIGNAL RELATED <-60 dBC in band, -5 dBm out; SIGNAL INDEPENDENT,<-60 dBm		
<-50 dBm, 26.5 - 27.5 and 28.5 - 29.5 GHz		
< -55 dBC for two carriers each at -10 dBm out		
±2.0 dB, 27.50 - 28.50 GHz out; ± 0.5 dB, 40 MHz BW		
Non-inverting		
26.155 GHz		
± 0.01 ppm maximum over temp internal reference; external reference input		
3 dBm, ± 3 dB, 75 ohms, External In or Internal Out		
100 MHz 1kHz 10kHz 100kHz 1MHz		
-70 -75 -80 -90 -110		
Selects Internal or External 10 MHz (Rear Panel DP3T Switch)		
Yellow LED, Indicates External 10 MHz Reference Selected		
Red LED, External Contact Closure		
Green LED		
BNC (female), 50Ω, (designated L-Band)		
DNC (remale), 5012, (designated L-band)		
$2.92 \text{ mm (female)}, 50\Omega$		
2.92 mm (female), 50Ω BNC (female), 75Ω Connector; Works for 50Ω or 75Ω		
2.92 mm (female), 50Ω BNC (female), 75Ω Connector; Works for 50Ω or 75Ω DB9 - NO or NC Contact Closure on Alarm		
2.92 mm (female), 50Ω BNC (female), 75Ω Connector; Works for 50Ω or 75Ω DB9 - NO or NC Contact Closure on Alarm 19 inch, Standard Chassis 1.75" high X 14.0" deep		
2.92 mm (female), 50Ω BNC (female), 75Ω Connector; Works for 50Ω or 75Ω DB9 - NO or NC Contact Closure on Alarm		
2.92 mm (female), 50Ω BNC (female), 75Ω Connector; Works for 50Ω or 75Ω DB9 - NO or NC Contact Closure on Alarm 19 inch, Standard Chassis 1.75" high X 14.0" deep 100-24 ±10% VAC, 47-63 Hz, 25 watts maximum		
2.92 mm (female), 50Ω BNC (female), 75Ω Connector; Works for 50Ω or 75Ω DB9 - NO or NC Contact Closure on Alarm 19 inch, Standard Chassis 1.75" high X 14.0" deep 100-24 ±10% VAC, 47-63 Hz, 25 watts maximum 50Ω 2.92 (RF), 75Ω BNC (L-Band)		
2.92 mm (female), 50Ω BNC (female), 75Ω Connector; Works for 50Ω or 75Ω DB9 - NO or NC Contact Closure on Alarm 19 inch, Standard Chassis 1.75" high X 14.0" deep 100-24 ±10% VAC, 47-63 Hz, 25 watts maximum		

2.0 Installation

2.1 Mechanical - The 2115-275-1845 consists of one RF PCB housed in a 1 RU (1 3/4 inch high) by 14 inch deep chassis. A switching, ± 12 , ± 24 , ± 5 VDC power supply provides power for the assemblies. The 2115-275-1845 can be secured to a rack using the 4 holes on the front panel. Figure 2.0 shows how the

2115-275-1845 is assembled.

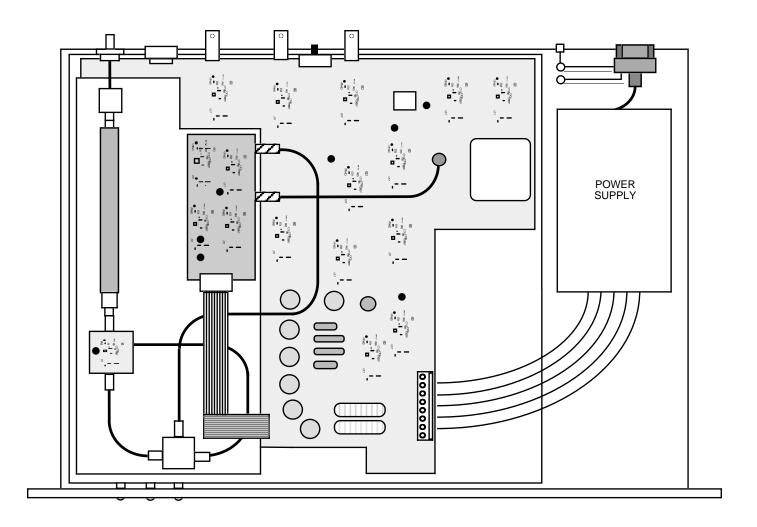

2115-275-1845 Mechanical Assembly FIGURE 2.0

2.2 Rear Panel Input/Output Signals - Figure 2.1 shows the input and output connectors on the rear panel.

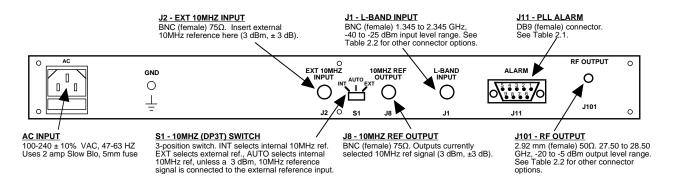


FIGURE 2.1 2115-275-1845 Rear Panel I/O's

TABLE 2.1 J11 Pinouts (DB9)		
Pin	Function	
1	Not Used	
2	Not Used	
3	Not Used	
4	Not Used	
5	GND	
6	Alarm Relay: Common	
7	Alarm Relay: Normally Open	
8	Not Used	
9	Alarm Relay: Normally Closed	

TABLE 2.2 Connector Options		
L-Band	RF	
BNC, 75Ω (STD)	SMA, 50Ω (STD)	
F-Type, 75Ω	SMA, 50Ω	
N-Type, 50Ω	SMA, 50Ω	
SMA, 50Ω	SMA, 50Ω	

2.3 Front Panel Indicators - The following are the front panel indicators.

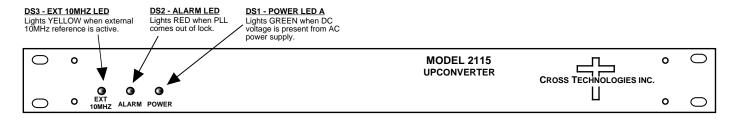


FIGURE 2.2 2115-275-1845 Front Panel Controls and Indicators

2.4 Installation / Operation

2.4.1 Installing and Operating the 2115-275-1845 Upconverter

- 1. Connect a -40 dBm to -25 dBm signal to L-BAND INPUT, J1 (Figure 2.1).
- 2. Connect the RF OUTPUT, J101, to the external equipment.
- 3. Connect $100-240 \pm 10\%$ VAC, 47 63 Hz to AC connector on the back panel.
- 4. Be sure DS1 (green, DC Power) is on and DS2 (red, Alarm) is off (Figure 2.2).
- 5. Select either INT (for internal 10MHz ref), AUTO (for internal 10MHz ref UNLESS a external 10MHz, 3 dBm signal is connected to J2), or EXT (for external 10MHz, 3 dBm ref that is inserted at J2) on rear panel switch S1 (Figure 2.1).
- 6. If EXT is selected or AUTO is selected and there is a 10MHz, 3 dBm signal at J2, check that DS3 (yellow, Ext 10MHZ) is on (Figure 2.2).
- 7. Check that a 10MHz, 3 dBm \pm 3 dB signal is present at the 10MHZ REF OUTPUT (J8) (Figure 2.1).
- 8. <u>AC Fuse</u> The fuse is a 5 mm X 20 mm, 2 amp slow blow (Type T) and is inserted in the far slot in the drawer below the AC input as shown in Figure 2.3. There is a spare fuse in the near slot. If a fuse continues to open, the power supply is most likely defective.

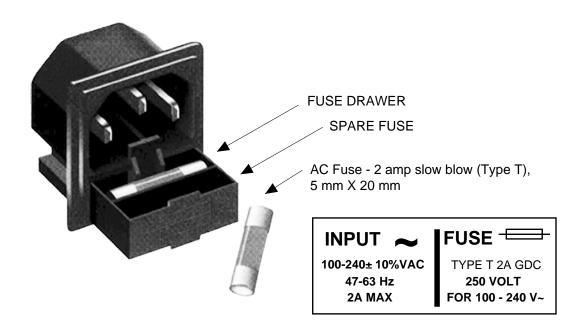


FIGURE 2.3 Fuse Location and Spare Fuse

2.5 Environmental Use Information

- **A. Rack-Mounting** To mount this equipment in a rack, please refer to the installation instructions located in the user manual furnished by the manufacturer of your equipment rack.
- **B. Mechanical Loading** Mounting of equipment in a rack should be such that a hazardous condition does not exist due to uneven weight distribution.
- C. **Elevated Operating Ambient Temperature** If installed in a closed or multi-unit rack assembly, the operating ambient temperature of the rack may be greater than room ambient temperature. Therefore, consideration should be given to Tmra (Maximum Recommended Ambient Temperature).
- **D.** Reduced Air Flow Installation of the equipment in a rack should be such that the amount of air flow required for safe operation of the equipment is not compromised. Additional space between units may be required.
- **E.** Circuit Overloading Consideration should be given to the connection of the equipment to the supply circuit and the effect that overloading of circuits could have on over current protection and supply wiring. Appropriate consideration of equipment name plate rating should be used, when addressing this concern.
- **F. Reliable Earthing** Reliable earthing of rack-mounted equipment should be maintained. Particular attention should be given to supply connections other than direct connection to the Branch (use of power strips).
- **G. Top Cover** There are no serviceable parts inside the product so, the Top Cover should not be removed. If the Top Cover is removed the ground strap and associated screw MUST BE REINSTALLED prior to Top Cover screw replacement. FAILURE TO DO this may cause INGRESS and/or EGRESS emission problems.



6170 Shiloh Road Alpharetta, Georgia 30005

(770) 886-8005 FAX (770) 886-7964 Toll Free 888-900-5588

WEB www.crosstechnologies.com E-MAIL info@crosstechnologies.com